



Indications

For examination uterine contents

Description

- The device consists of a clear, flexible outer sheath 250mm and 3.0 mm OD (outside diameter), marked with 9 sounding marks.
- •Distal Type are available Open or Closed depending on a physician and patient's situation.
- The device draws cell through a distal collection port by means of a vacuum, created when the inner plunger is pulled through the outer sheath.

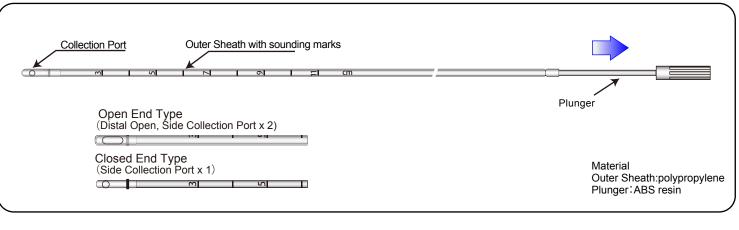





2. Once in position, discontinue any traction applied.
Then, hold the sheath in one hand, and smoothly draw back the plunger to the stop, thus creating a vacuum within the sheath.



Upon completion of the rotating/stroking motions, leave the plunger withdrawn and remove the entire device from the canal.

[Endometrial Specimen Collection]

- Open End Type
 Express the contents
- Closed End Type
 Snip the distal end of the sheath immediately proximal to the distal opening with a sterile pair of scissors.

SPECIFICATIONS TYPE and SIZE Open End Type 2.5×3.0×250mm Closed End Type 2.5×3.0×250mm Package 10 pcs/BOX with EOG sterilized Expired date on Label •Please read carefully IFU before use.

Hakk o

Hakko Co.,Ltd.

and the fundus of the uterus.

in and out between the internal cervical os

[Head Office] 3055 O-aza Toguraonsen,Chikuma-shi,Nagano,JAPAN [Factory site] 1490 O-aza Isobe, chikuma-shi, Nagano, JAPAN [Head Sales] Hongou 3-chome,Bunkyo-ku,Tokyo, JAPAN Please visit http://www.hakko-medical.com